





Compensatory Magnetic Oscillators

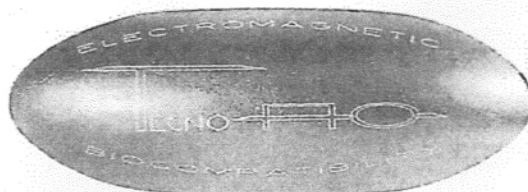

FOR CELLULAR PHONES
0.8/0.9 GHz AND 1.8/1.9 GHz AND TRI-BAND

AUTONOMOUS OSCILLATORS · TECHNOLOGY FOR ELECTROMAGNETIC BIOCOMPATIBILITY

TECHNOLOGY TO CORRECT THE BIOLOGICAL EFFECTS OF RADIATING

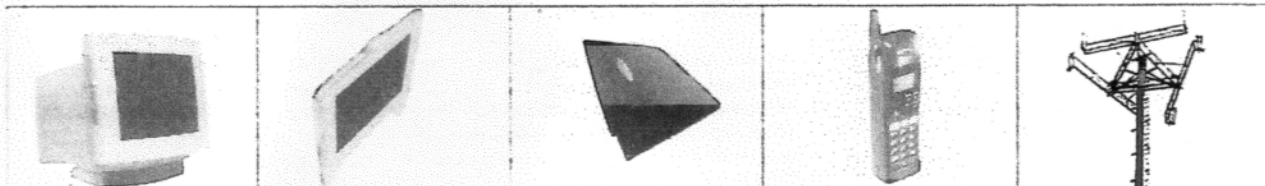

DEVICES SUCH AS COMPUTERS / TV SETS / PORTABLE COMPUTERS /
LCD FLAT SCREENS / CELLULAR PHONES / CELLULAR TELEPHONY BASE
STATIONS

ISSUED BY
THE INTERNATIONAL CENTRE OF RESEARCH
IN ELECTROMAGNETIC BIOPHYSICS-TECNOLAB

INTERNATIONAL PATENTS




TECNOLAB'S RESEARCH HAS ENABLED THE CREATION OF
ELECTROMAGNETIC BIOCOMPATIBILITY BETWEEN ELECTROMAGNETIC
STRESSING FIELDS AND LIVING SYSTEMS USING THE TECHNOLOGY OF
MAGNETIC COMPENSATION EMISSION



CMO BIOPROTECTION IS AN APPLICATION OF THE PRECAUTIONARY
PRINCIPLE, BASED ON BIOLOGICAL PROOFS FROM TEN YEARS OF STUDIES
IN UNIVERSITIES ON ANIMALS AND HUMANS


SOME BIOLOGICAL EFFECTS SHOWING CMO ELECTROMAGNETIC PROTECTIVE ACTION

EMBRYONIC MORTALITY

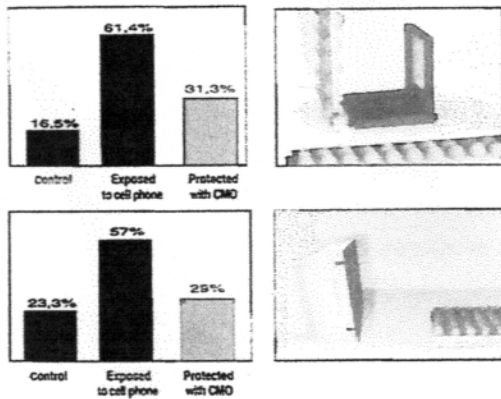


(Bioelectromagnetics 1997 ; BEMS 1998 ; NIR 2000 ; SPPCR 2001 ; Indoor and Built Environment 2001)

ELECTROMAGNETIC WAVE SPECTRUM

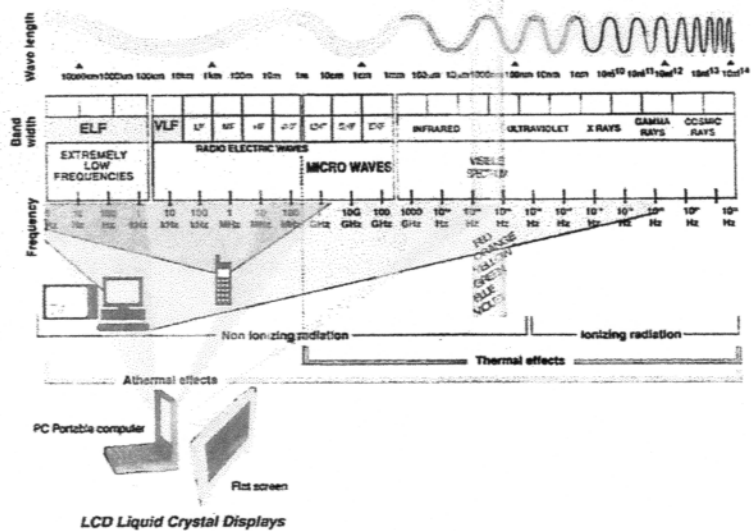


CALCIUM CONCENTRATION IN BRAIN CELLS

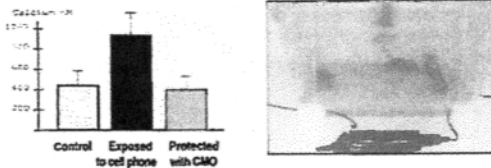


CALCIUM : AN ABNORMAL VARIATION OF INTRACELLULAR CALCIUM CONCENTRATION MAY LEAD TO NERVOUS, IMMUNE AND HORMONAL DYSFUNCTION. MICE EXPOSURE TO CELL PHONES IS STRESSFUL SINCE IT INCREASES CALCIUM CONCENTRATION IN BRAIN CELLS. CMO MAINTAINS NORMAL CALCIUM CONCENTRATION IN BRAIN CELLS. (SPPCR-IRPA 2001)

MELATONIN ANTISTRESS HORMONE AND IMMUNE SYSTEM ENHANCER

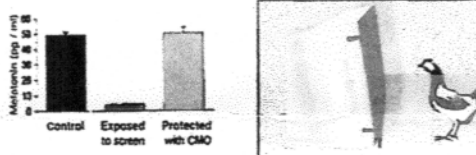



MELATONIN : A DECREASE OF THE PRODUCTION OF MELATONIN (PINEAL HORMONE) MAY DEPRESS THE IMMUNE SYSTEM. ADULT ANIMAL EXPOSURE TO VDU (TV AND COMPUTER SCREENS) IS STRESSFUL SINCE IT INDUCES A DECREASE OF (MELATONIN AND CORTICOSTERONE) HORMONES LEVELS. CMO MAINTAINS NORMAL ALL HORMONAL LEVELS. (EBEA 1996 ; Bioelectromagnetics 1997 ; BEMS 1998 ; NIR 2000 ; Radioprotecao 2001)

DNA : THE FORMATION OF MICRONUCLEI IN CELLS MEANS CELL DYSFUNCTION, CELL DEATH OR INDUCTION OF CANCER. CMO REDUCES SIGNIFICANTLY THE FORMATION OF MICRONUCLEI. (EBEA 2001)

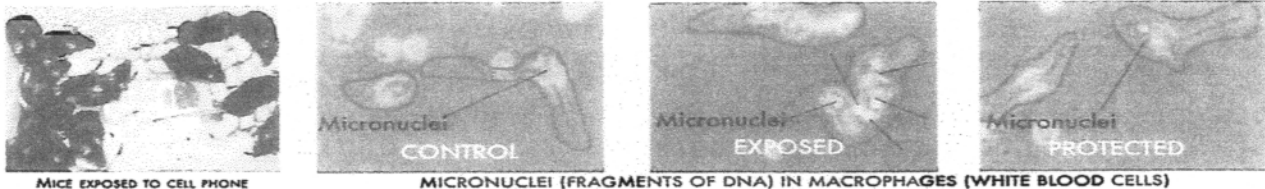


ALL SCIENTIFIC STUDIES ABOUT CMO ARE ON INTERNET : www.electromagnetic-biocompatibility.com
AND IN THE BOOK : "ELECTROMAGNETIC BIOCOMPATIBILITY. ELECTROMAGNETIC FIELDS AND LIVING SYSTEMS ..."

EMBRYONIC MORTALITY

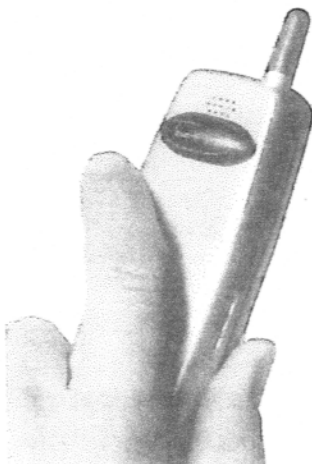

CHICKEN EMBRO EXPOSED TO CELL PHONE



Manufacturer guarantee
this device is guaranteed for two years
in normal conditions of use.

CMO OSCILLATOR

FOR CELLULAR PHONE (0.8/0.9
GHZ AND 1.8/1.9 GHZ AND TRI-BAND)
TO COMPENSATE FOR THE
BIOLOGICAL EFFECTS OF THEIR
ELECTROMAGNETIC FIELDS.

Instructions for use

Remove the colour slip from the self adhesive patch and fix the CMO oscillator on a flat surface of your cellular phone. Caution : Do not expose your cell phone equipped with the oscillator to temperatures above 65°C.